


HILIC Separation of Hydroxypiperidine and Impurities

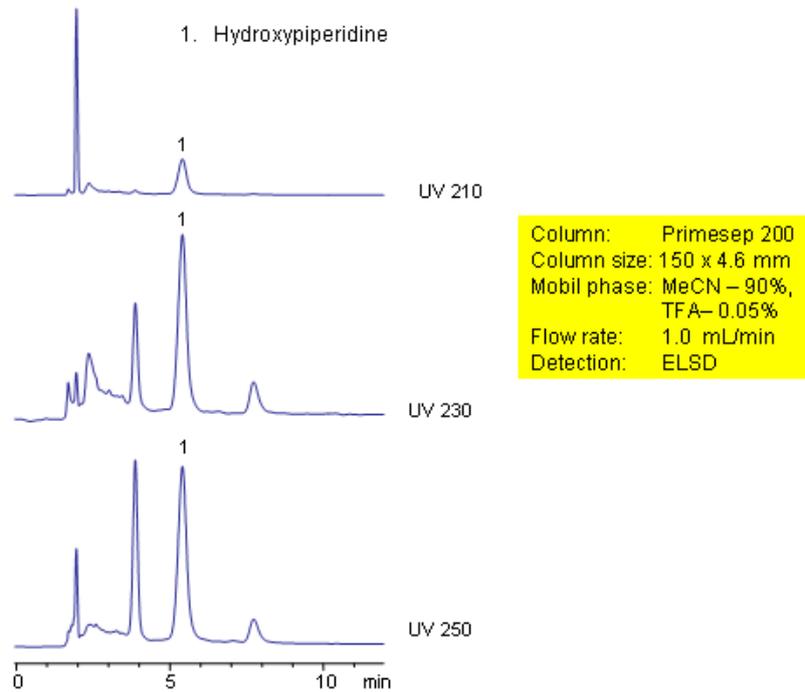

Primesep 200 mixed-mode column is used in HILIC/cation-exchange mode to separate hydroxypiperidine and related impurities. Compounds are monitored by ELSD in the presence of trifluoroacetic acid in the mobile phase.

Method Parameters

Detection	ELSD Detection
-----------	----------------

Quelle: <https://sielc.com/Application-HILIC-Separation-of-Hydroxypiperidine-and-Impurities>