
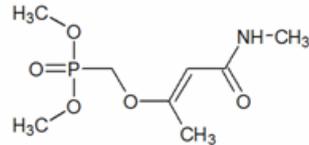


HPLC Analysis of Monocrotopos

Column: Obelisc R
Dimensions: 150 x 4.6mm
Mobile Phase: 50% MeCN
Buffer: 20mM AmFm pH 3.0
Flow: 1.0 ml/min
Detection: UV 250 nm

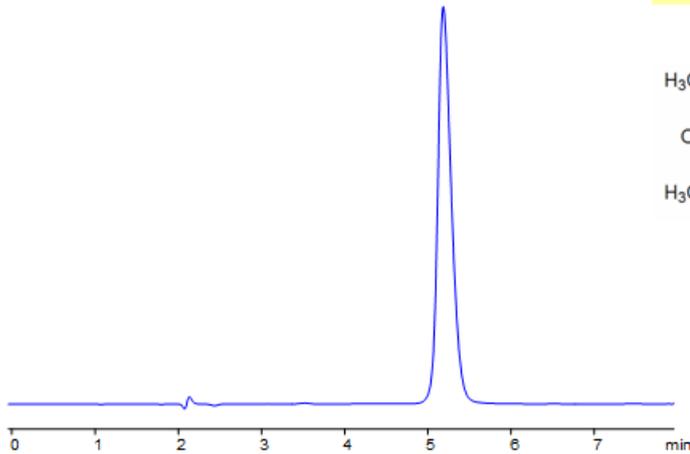

SIELC has developed the Obelisc™ columns, which are mixed-mode and utilize Liquid Separation Cell technology (LiSC™). These cost-effective columns are the first of their kind to be commercially available and can replace multiple HPLC columns, including reversed-phase (RP), AQ-type reversed-phase, polar-embedded group RP columns, normal-phase, cation-exchange, anion-exchange, ion-exclusion, and HILIC (Hydrophilic Interaction Liquid Chromatography) columns. By controlling just three orthogonal method parameters - buffer concentration, buffer pH, and organic modifier concentration - users can adjust the column properties with pinpoint precision to separate complex mixtures.

Method Parameters

Column	Obelisc R, 4.6x150 mm, 5 µm, 100 Å
Mobile Phase	MeCN – 50%
Buffer	AmFm pH 3.0- 20 mM
Flow Rate	1.0 mL/min
Detection	UV, 250 nm

Quelle: <https://sielc.com/Application-HPLC-Analysis-of-Monocrotopos>