


HPLC Method for Analysis of Azor

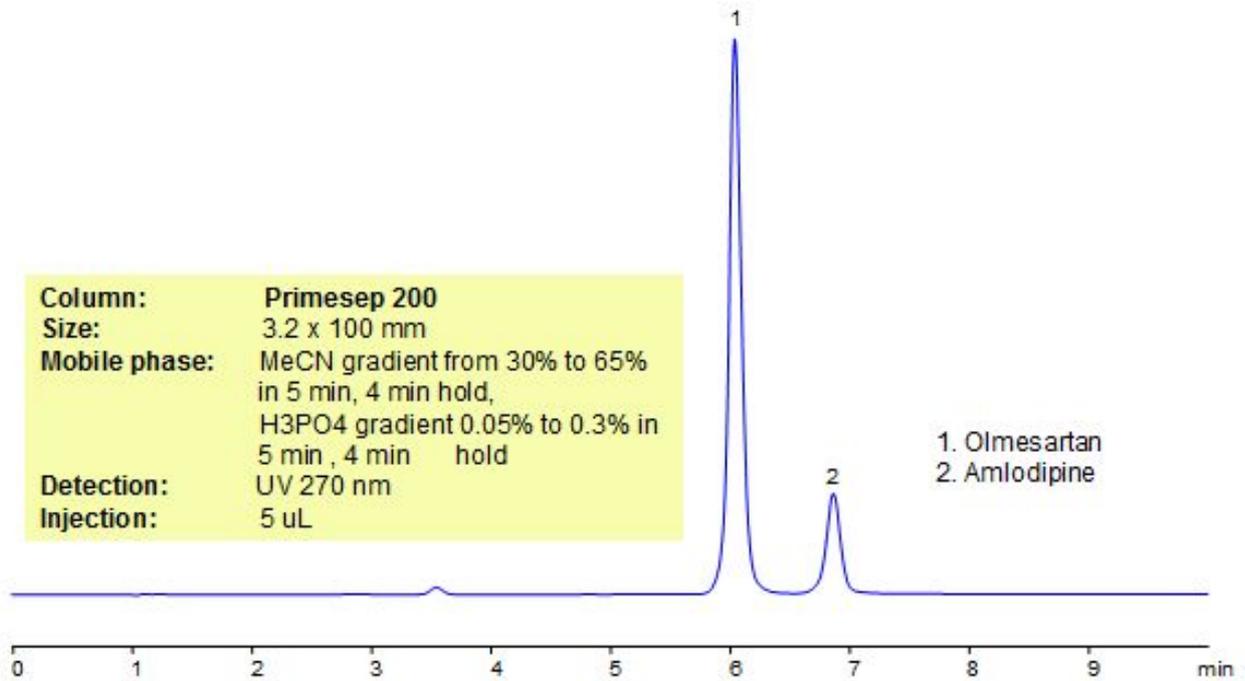

Method Parameters

Column	Primesep 200, 3.2x100 mm, 5 µm, 100 Å
Mobile Phase	Gradient MeCN – 30/65%
Buffer	Gradient H3PO4 – 0.05-0.3%, 5 min, 4 min hold
Flow Rate	0.5 mL/min
Detection	UV, 270 nm

Quelle: <https://sielc.com/HPLC-Method-Analysis-Azor>