


## HPLC Method for Analysis of Insulin on BIST™B+ Column

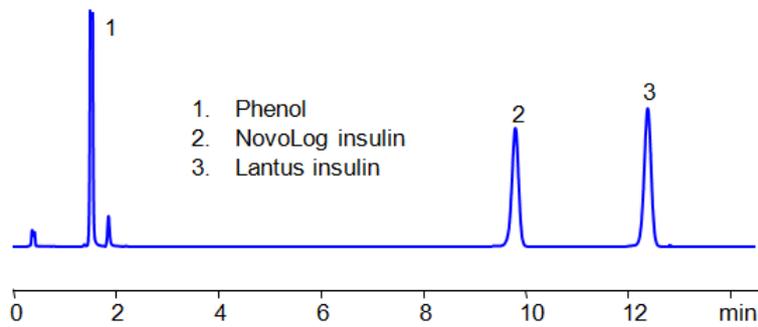

**Column:** BIST™ B+  
**Size:** 4.6 × 150mm, 5 µm  
**Flow:** 1.0 mL/min  
**Mobile phase:** Gradient MeCN – 75 → 55%, 15 min  
**Buffer:** H<sub>2</sub>SO<sub>4</sub> – 0.2%  
**Detection:** UV 210 nm

### Method Parameters

<b>Mobile Phase</b>	MeCN Gradient
<b>Buffer</b>	H <sub>2</sub> SO <sub>4</sub> – 0.2%
<b>Flow Rate</b>	1.0 mL/min
<b>Detection</b>	UV 210 nm

Quelle: <https://sielc.com/hplc-method-for-analysis-of-insulin>