


HPLC Method for Analysis of Warfarin on Newcrom R1 Column

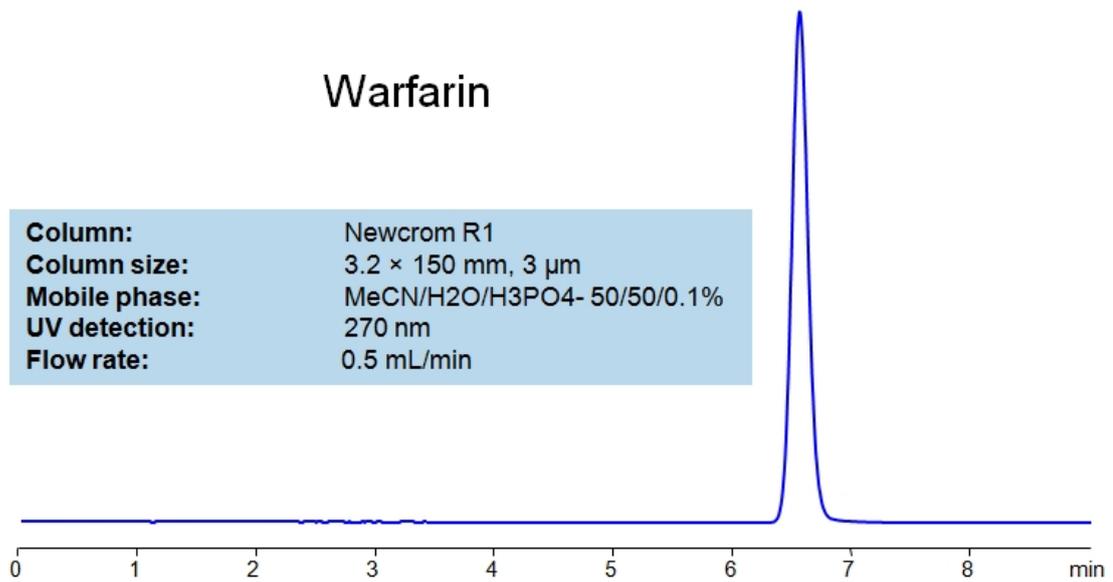

Method Parameters

Column	Newcrom R1, 3.2 x 150 mm, 3 µm, 100 Å, dual ended
Mobile Phase	MeCN – 50%
Buffer	Phosphoric Acid
Flow Rate	0.5 mL/min
Detection	UV 270 nm

Quelle: <https://sielc.com/hplc-method-for-analysis-of-warfarin>