


HPLC Method for Separation of Urea and Hydrogen Peroxide

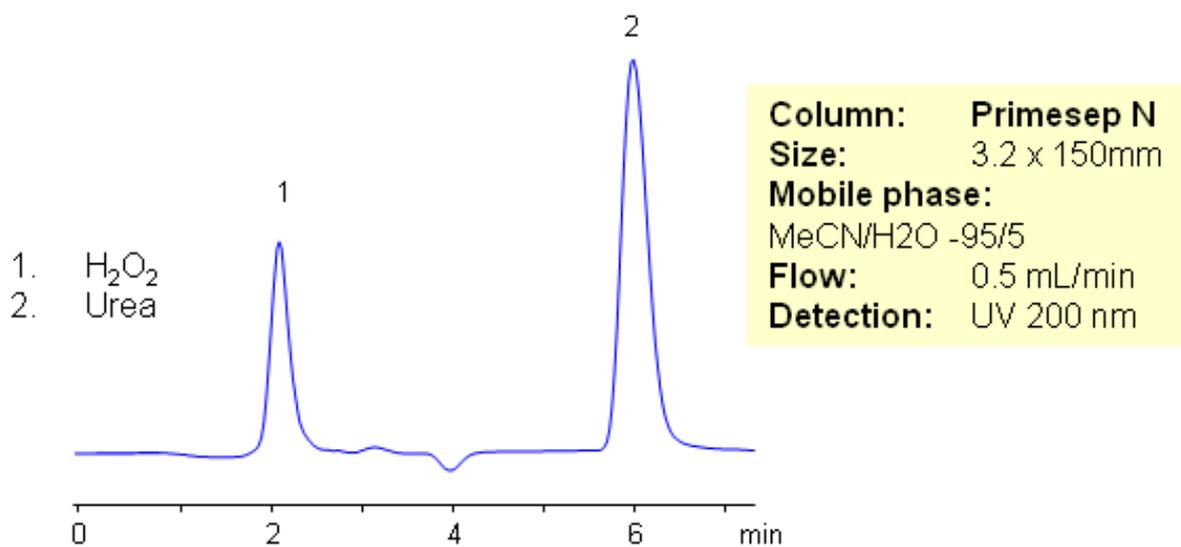

Urea and carbamide are separated by HILIC HPLC on Primesep N column. Both compounds can be monitored at low UV – 200 nm. Method can be used for determination and quantitation of hydrogen peroxide and urea in various matrices.

Method Parameters

Detection	UV Detection
-----------	--------------

Quelle: <https://sielc.com/Application-HPLC-Method-For-Separation-of-Urea-and-Hydrogen-Peroxide>