



HPLC Retention of Terbufos on Obelisc N Mixed-Mode Column

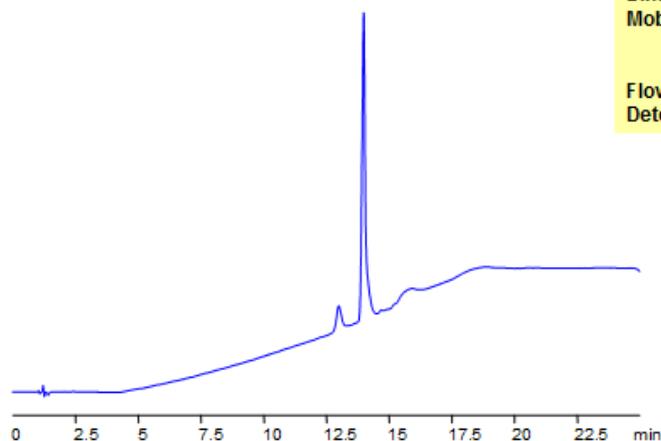

Column: Obelisc R
Dimensions: 150 x 2.1mm
Mobile Phase: MeCN gradient from 10% to 70% in 15 min, 7 min hold. AmAc pH 4.5 from 20 mM to 50 mM in 15 min, 7 min hold
Flow: 0.4 mL/min
Detection: UV 250 nm

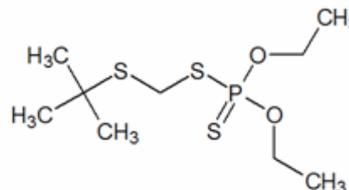

Method Parameters

Column	Obelisc R, 2.1x150 mm, 5 µm, 100 Å
Mobile Phase	Gradient MeCN – 10-70%, 15 min, 7 min hold
Buffer	Gradient AmAc pH 4,5- 20-50 mM, 15 min, 7 min hold
Flow Rate	0.4 mL/min
Detection	UV, 250 nm

Quelle: <https://sielc.com/Application-HPLC-Retention-of-Terbufos-on-Obelisc-N-Mixed-Mode-Column>