


HPLC Separation of Guanidine and Benzoic Acids on Primesep 100 Column

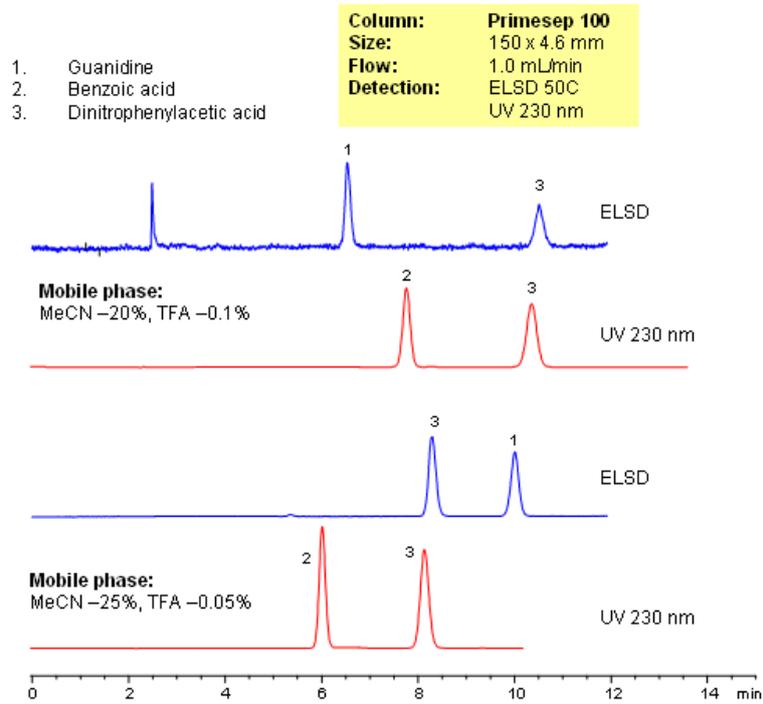

Method Parameters

Column	Primesep 100, 4.6x150 mm, 5 µm, 100 Å
Mobile Phase	MeCN/H ₂ O
Buffer	TFA
Flow Rate	1.0 mL/min
Detection	UV, 230 nm, ELSD

Quelle: <https://sielc.com/Application-HPLC-Separation-of-Guanidine-and-Benzoic-Acids-on-Primesep-100-Column>