
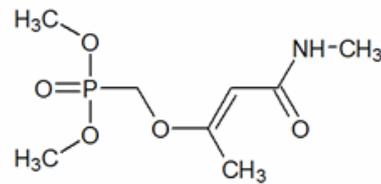


Monocrotophos Separation on Obelisc and Primesep Mixed-Mode HPLC Columns

Dimensions: 150 x 2.1 mm
Mobile Phase: MeCN gradient from 10% to 70% in 15 min, 7 min hold. AmAc pH 4.5 from 20 mM to 50 mM in 15 min, 7 min hold
Flow: 0.4 ml/min
Detection: UV 250 nm

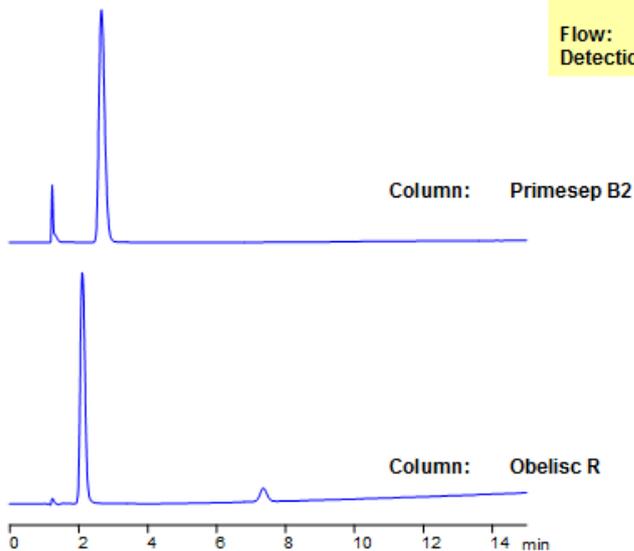

SIELC has developed the Obelisc™ columns, which are mixed-mode and utilize Liquid Separation Cell technology (LiSC™). These cost-effective columns are the first of their kind to be commercially available and can replace multiple HPLC columns, including reversed-phase (RP), AQ-type reversed-phase, polar-embedded group RP columns, normal-phase, cation-exchange, anion-exchange, ion-exclusion, and HILIC (Hydrophilic Interaction Liquid Chromatography) columns. By controlling just three orthogonal method parameters - buffer concentration, buffer pH, and organic modifier concentration - users can adjust the column properties with pinpoint precision to separate complex mixtures.

Method Parameters

| | |
|---------------------|--|
| Column | Obelisc R, 2.1x150 mm, 5 µm, 100 Å |
| Mobile Phase | Gradient MeCN – 10-70%, 15 min, 7 min hold |
| Buffer | Gradient AmAc pH 4,5- 20-50 mM, 15 min, 7 min hold |
| Flow Rate | 0.4 mL/min |
| Detection | UV, 250 nm |

Quelle:

<https://sielc.com/Application-Monocrotophos-Separation-on-Obelisc-and-Primesep-Mixed-Mode-HPLC-Columns>