


## Separation of Vitamins in Mixed-Mode HPLC

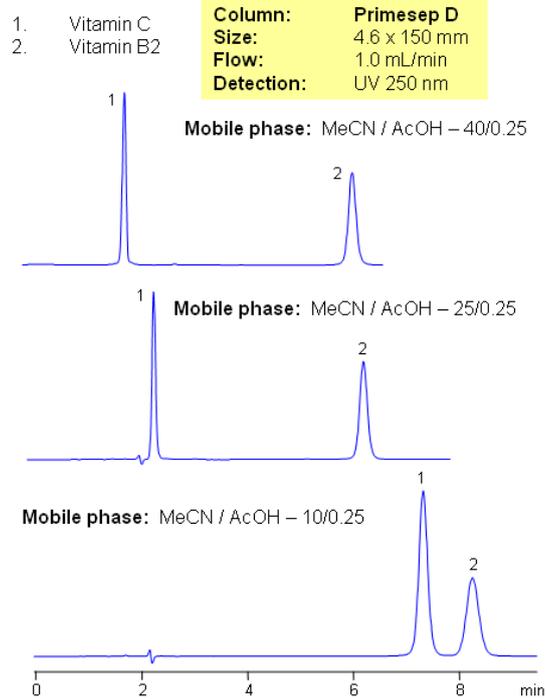

Separation of Vitamin B2 and Vitamin C is demonstrated on a Primesep D mixed-mode column. This column can be used for analysis of other hydrophobic or neutral vitamins and supplements.

### Method Parameters

<b>Column</b>	Primesep D , 4.6x150 mm, 5 µm, 100 Å
<b>Mobile Phase</b>	MeCN/H <sub>2</sub> O
<b>Buffer</b>	Acetic Acid
<b>Flow Rate</b>	1.0 mL/min
<b>Detection</b>	UV, 250 nm

Quelle: <https://sielc.com/Application-Separation-of-Vitamins-in-Mixed-Mode-HPLC>