


## HPLC Analysis of 18 Amino Acids on Amaze HD Column

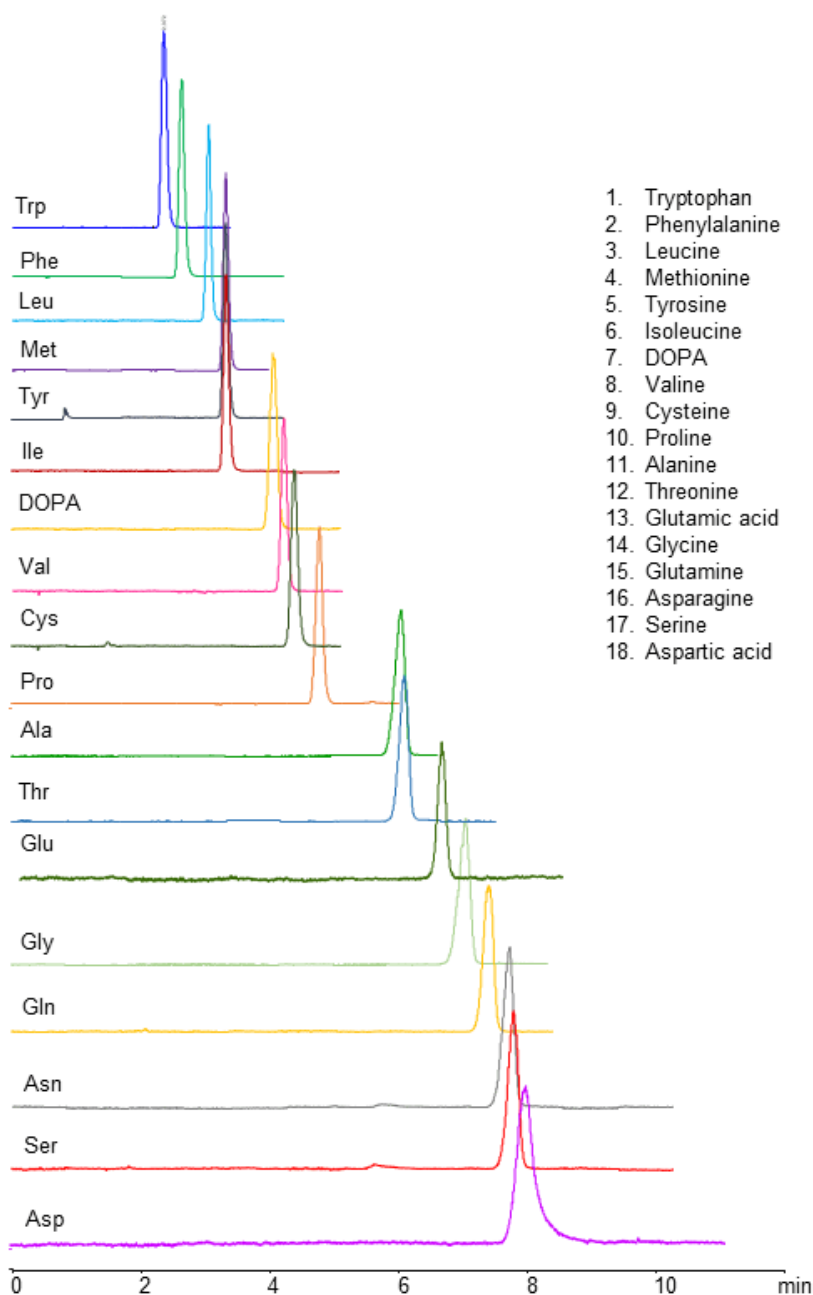

Column: Amaze HD

Separation Modes: HILIC, cation-exchange

Column Dimensions: 3.0x100 mm, 5  $\mu$ m, 100A

Mobile Phase: 80% ACN with 20 mM AmFm pH 3

Detection: ELSD, 45°C

Sample: 0.5-0.8 mg/ml

Injection: 3  $\mu$ l

Flow rate: 0.6 ml/min

Compounds: Tryptophan, Phenylalanine, Leucine, Methionine, Tyrosine, Isoleucine, DOPA, Valine, Cysteine, Proline, Alanine, Threonine, Glutamic acid, Glycine, Glutamine, Asparagine, Serine, Aspartic acid

Ihr Ansprechpartner:

AugustaChrom – Dr. Roland Kießwetter

info@hplc-shop.de

Tel. +49 821 599 783 70