


# HPLC Separation of Guanidine and Benzoic Acids on Primesep 100 Column

<https://sielc.com/Application-HPLC-Separation-of-Guanidine-and-Benzoic-Acids-on-Primesep-100-Column>

## Chromatogram

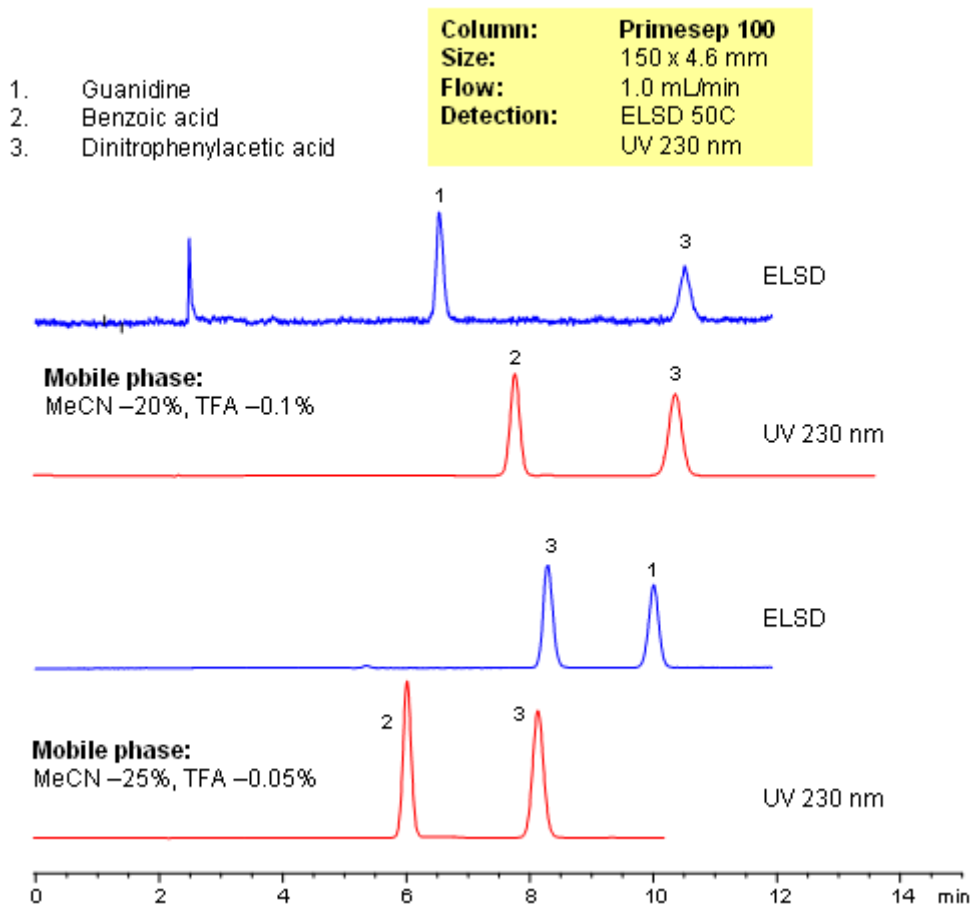

## Method Parameters

Mobile Phase	MeCN/H <sub>2</sub> O
Buffer	TFA
Flow Rate	1.0 ml/min
Detection	UV, 230 nm, ELSD
Class of Compounds	Acid, Hydrophilic, Ionizable
Analyzing Compounds	Guanidine, Benzoic acid, Dinitrophenylacetic Acid

## HPLC Column Used

**Primesep 100, 4.6x150 mm, 5 µm, 100A**

[Order this column at hplc-shop.de →](#)